

Applicant(s): Henry A. Hill

## MEASUREMENT AND COMPENSATION OF ERRORS IN INTERFEROMETERS


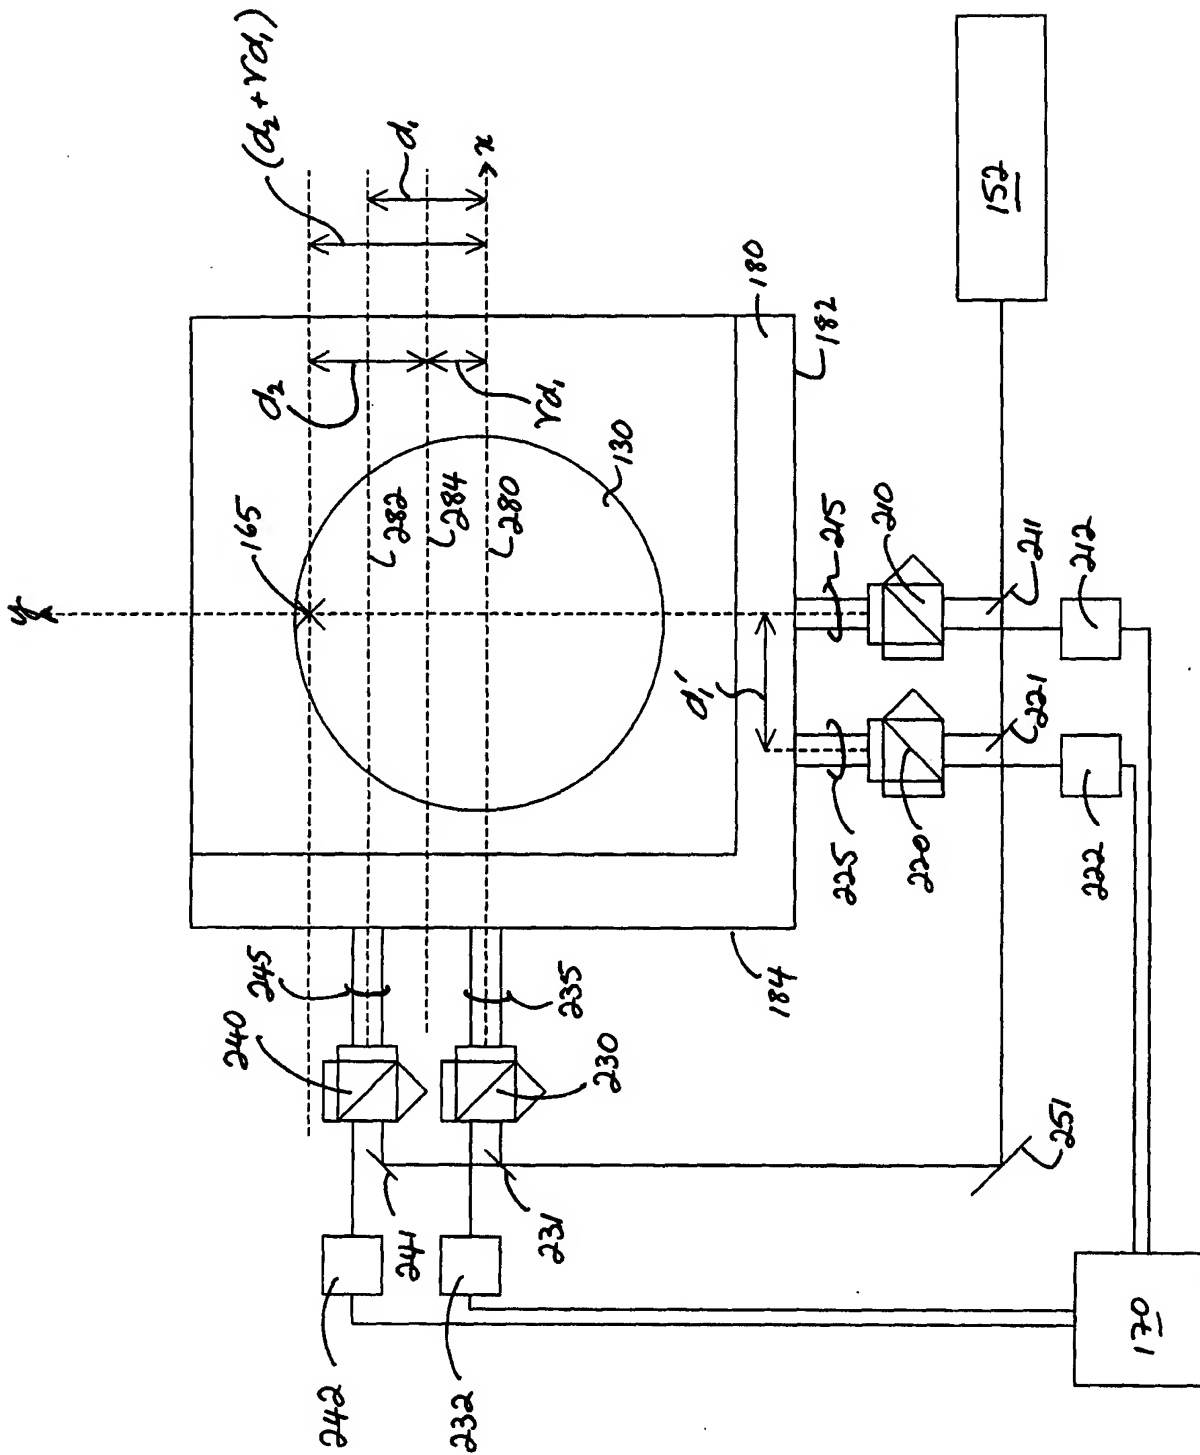


FIG. 2

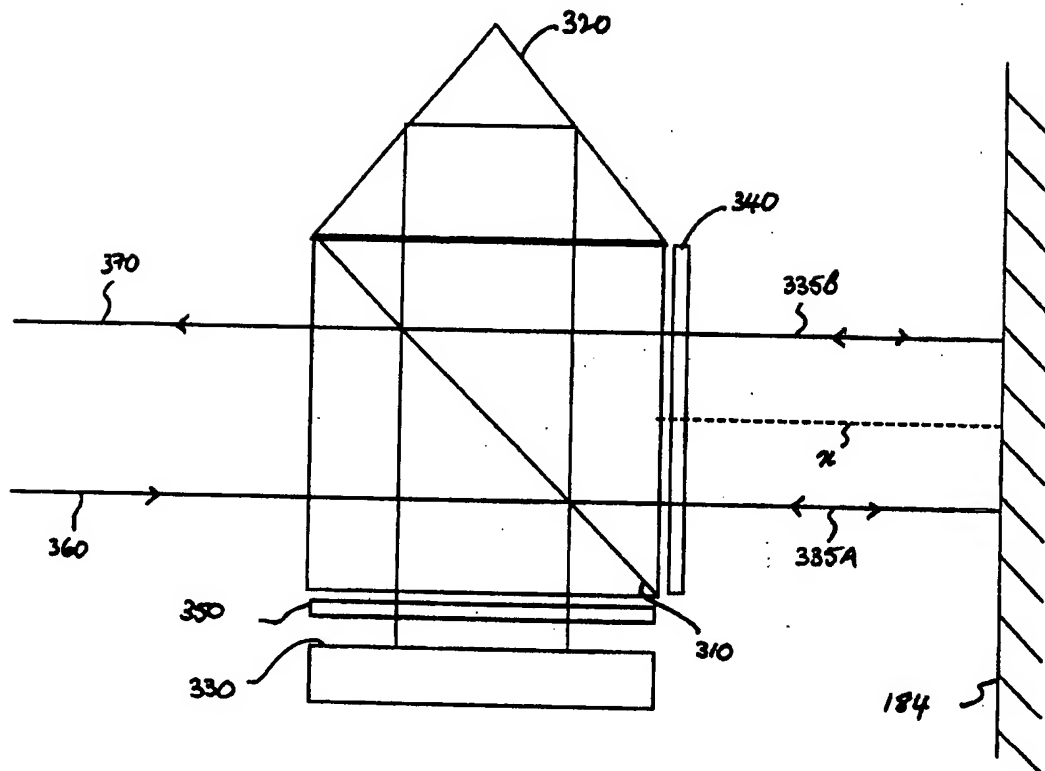

300

FIG. 3




FIG. 4

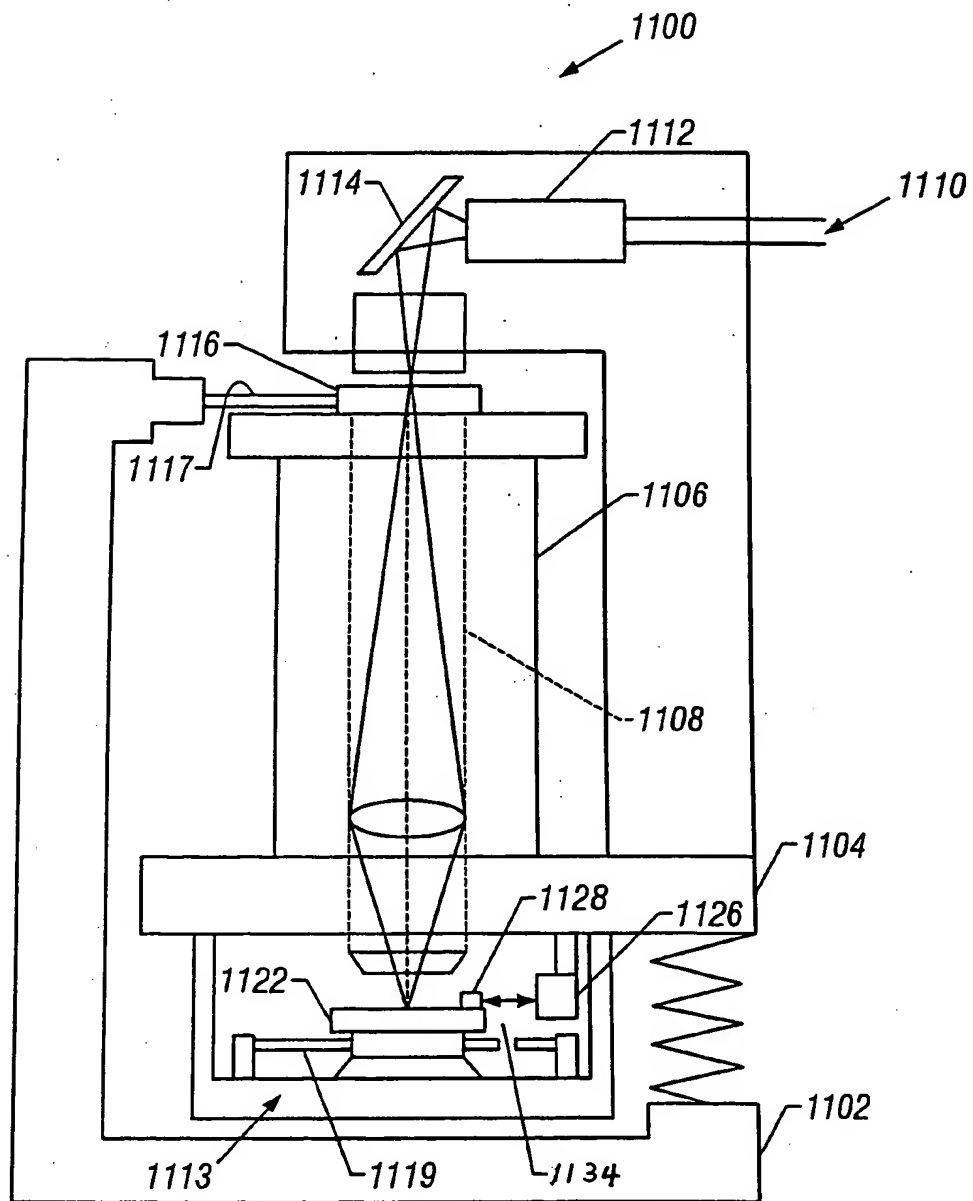


FIG. 5

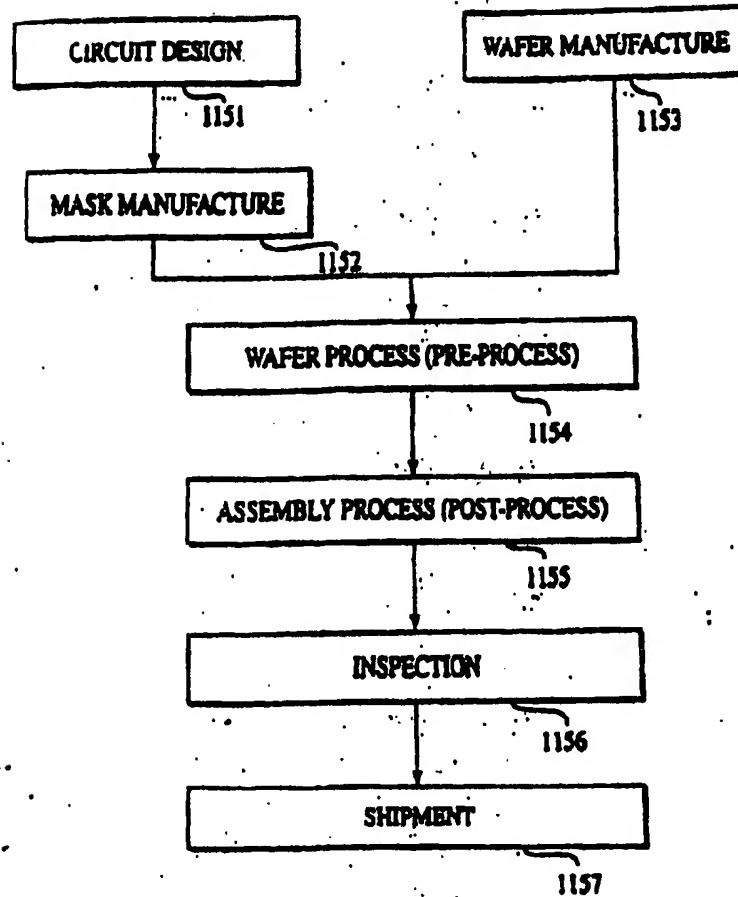


FIG. 6(a)

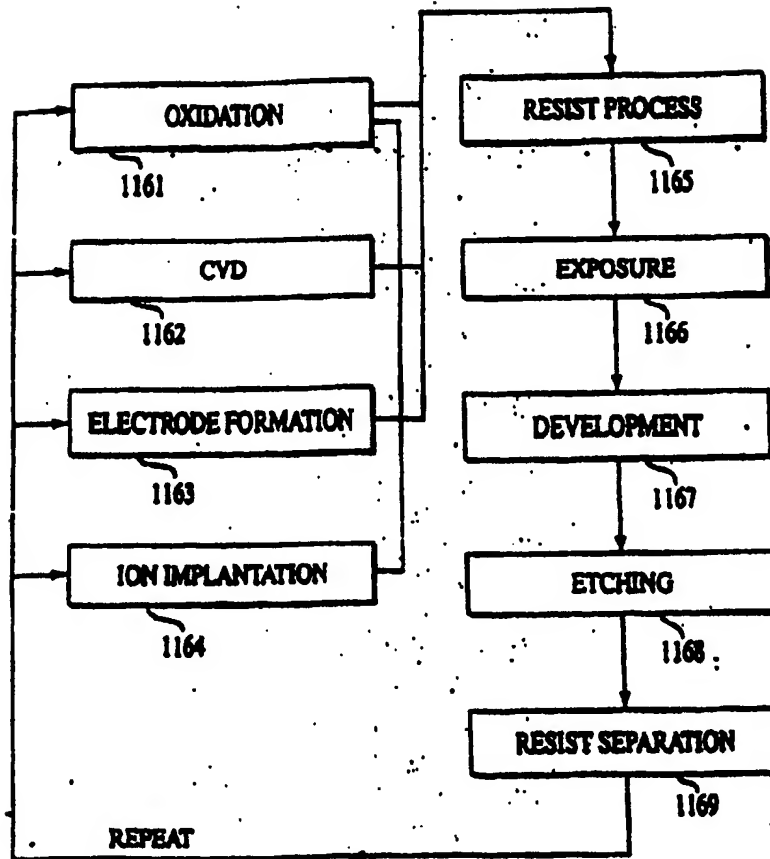


FIG. 6(b)

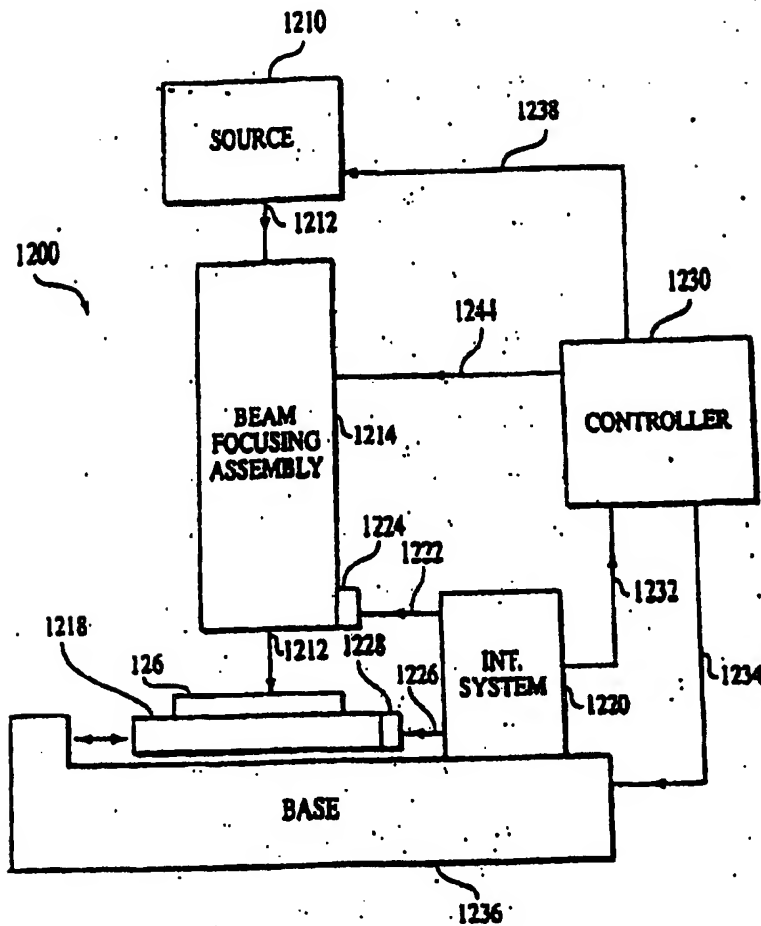


FIG. 7